

WO 01/14909

PCT/FR00/02370

1/2

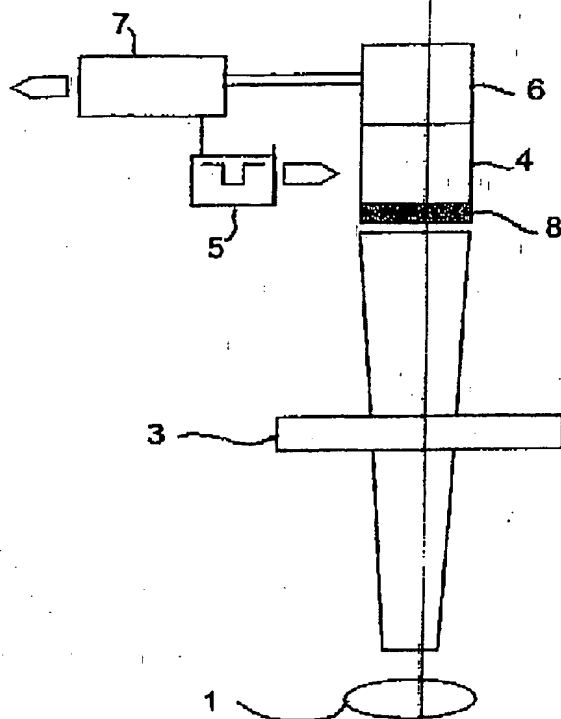


Fig.1

Primary source 1	Calibration source 5	turned off	turned on
"	"	"	"
Source principale 1	Source calibration 5	éteinte	allumée

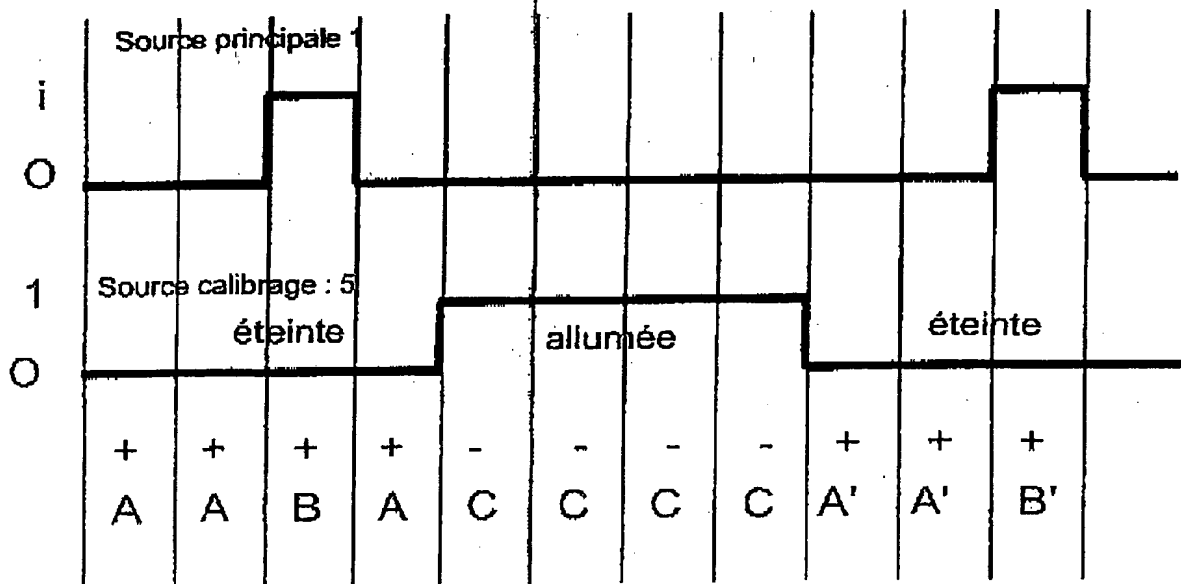


Fig.2

WO 01/14909

2/2

PCT/FR00/02370

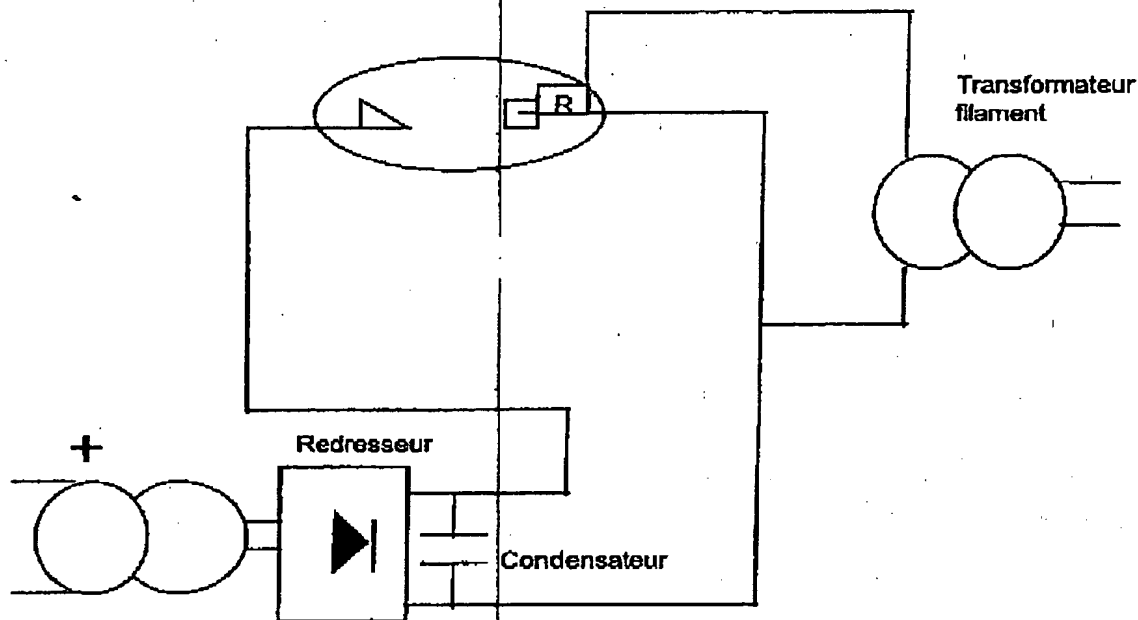


Fig.3B

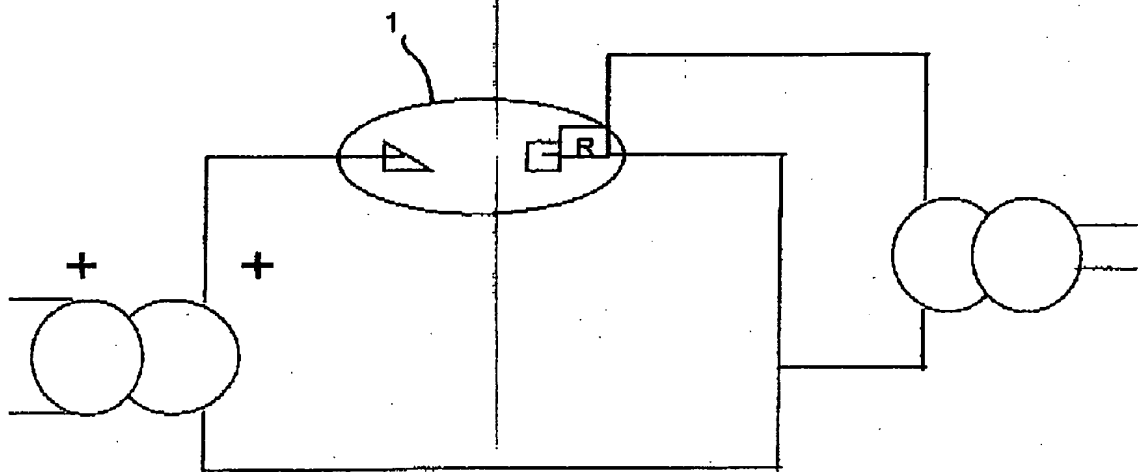


Fig. 3A

Transformateur filament	=	Filament transformer
Redresseur	=	Rectifier
Condensateur	=	Capacitor